RX-MD03-0224

Status	Date	Size	Transfer	Category	Phase
Curation S12-225	220523	29.1	MD03-G0620,SG45b2,S12-225	1	ol,lpx

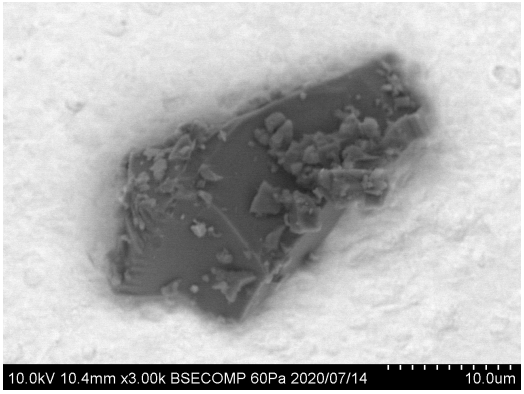

20200714/Au13_SEM/image/03_MD03-G0620_bse.bmp

SAMPLE : RX-MD03-0224
PREID : MD03-G0620
PROCESS : BSE
OPERATOR : Nishimura
COMMENT :

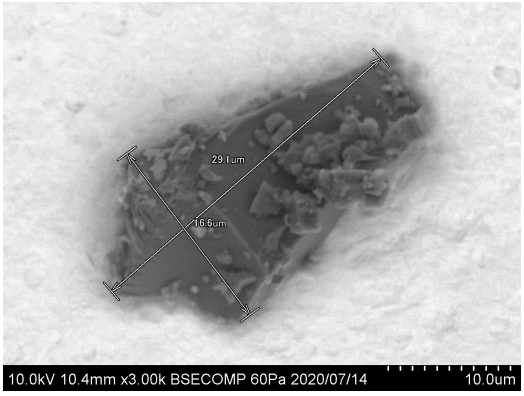

20200714/Au13_SEM/image/20_MD03-G0620_bse_scaled.bmp

SAMPLE : RX-MD03-0224
PREID : MD03-G0620
PROCESS : BSE
OPERATOR : Nishimura
COMMENT : scaled

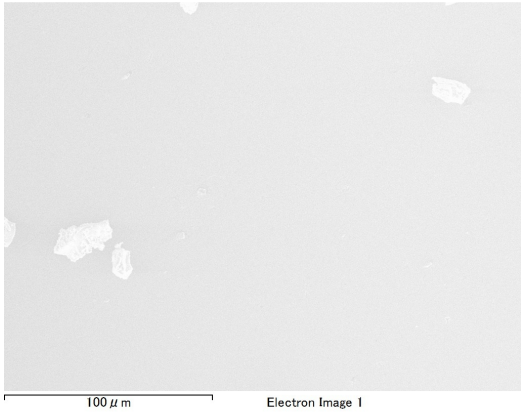

20200227/RX-MD03_SEM/eds/10_MD03-G0620_EDSatMD03.docx

SAMPLE : RX-MD03-0224
PREID : MD03-G0620
PROCESS : EDS at MD03
OPERATOR : Iwamae
COMMENT : No EDS data

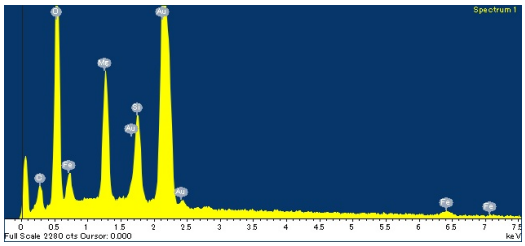

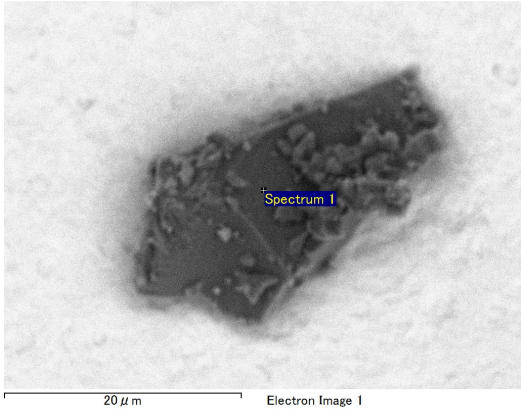

20200714/Au13_SEM/eds/02_MD03-G0620_EDSatAu13s2.docx

SAMPLE : RX-MD03-0224
PREID : MD03-G0620
PROCESS : EDS at Au13s2
OPERATOR : Nishimura
COMMENT :

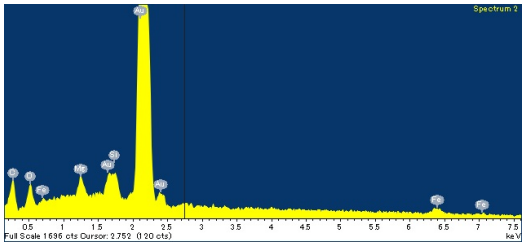
Spectrum 2
Cl
Cl
Cu
Cu
Cu
Au
Au
Au
Au
0.5 1 1.5 2 2.5 3 3.5 4 4.5 5 5.5 6 6.5 7 7.5
Full Scale 1696 cts Cursor: 2.752 (120 cts)
keV

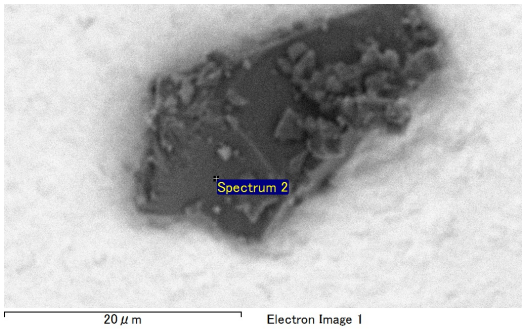
Spectrum 2
20 μm
Electron Image 1

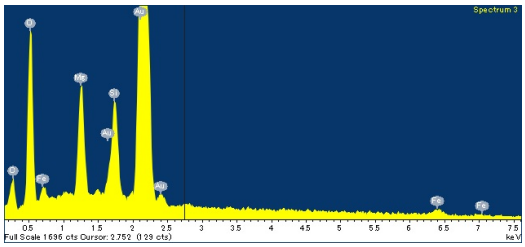
Spectrum 3
Cl
Cl
Cu
Cu
Cu
Au
Au
Au
Au
0.5 1 1.5 2 2.5 3 3.5 4 4.5 5 5.5 6 6.5 7 7.5
Full Scale 1696 cts Cursor: 2.752 (129 cts)
keV

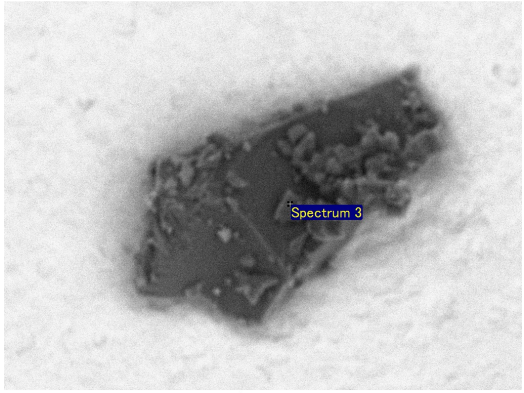
Spectrum 3
20 μm
Electron Image 1

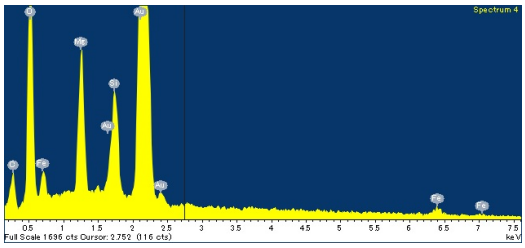
Spectrum 4
Cl
Cl
Cu
Cu
Cu
Au
Au
Au
Au
0.5 1 1.5 2 2.5 3 3.5 4 4.5 5 5.5 6 6.5 7 7.5
Full Scale 1696 cts Cursor: 2.752 (116 cts)
keV

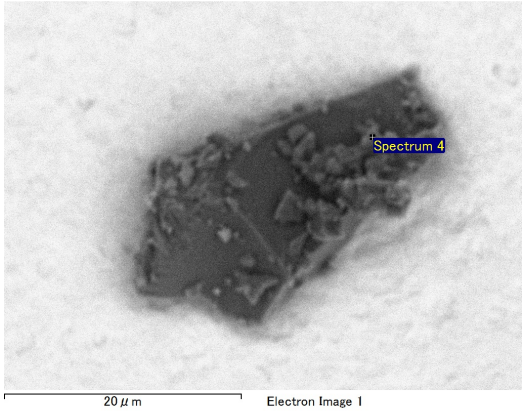
Spectrum 4
20 μm
Electron Image 1

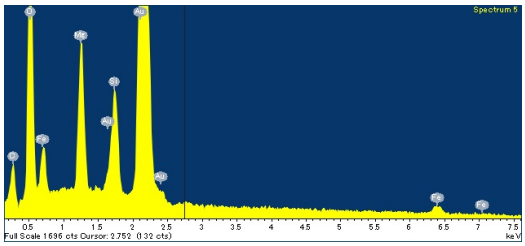
Spectrum 5
Cl
Cl
Cu
Cu
Cu
Au
Au
Au
Au
0.5 1 1.5 2 2.5 3 3.5 4 4.5 5 5.5 6 6.5 7 7.5
Full Scale 1696 cts Cursor: 2.752 (132 cts)
keV

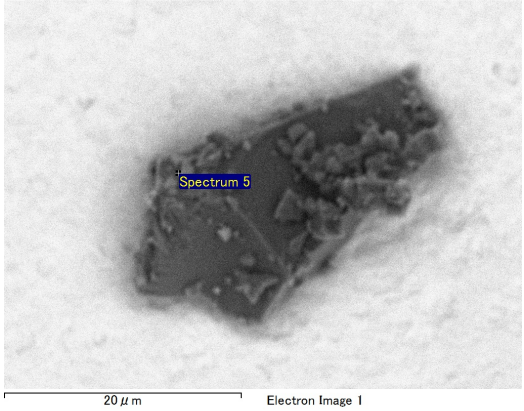
Spectrum 5
20 μm
Electron Image 1

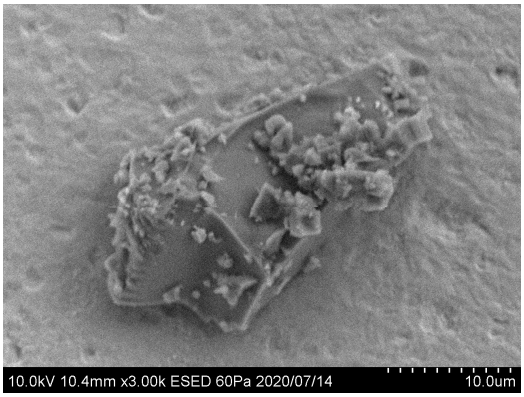

20200714/Au13_SEM/image/04_MD03-G0620_esed.bmp

SAMPLE : RX-MD03-0224
PREID : MD03-G0620
PROCESS : ESED
OPERATOR : Nishimura
COMMENT :

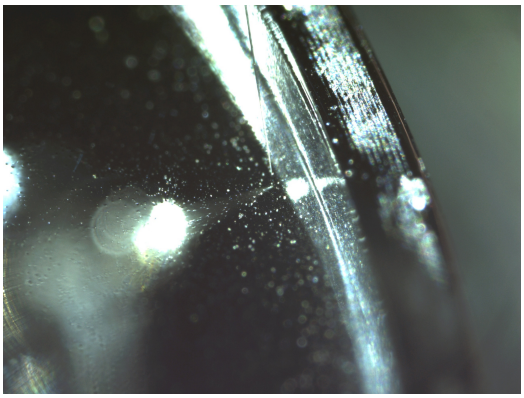

20200713/toAu13/nikon/01_MD03-G0620_pickup.bmp

SAMPLE : RX-MD03-0224
PREID : MD03-G0620
PROCESS : pickup from MD03
OPERATOR : Yoshitake, Nishimura
COMMENT :

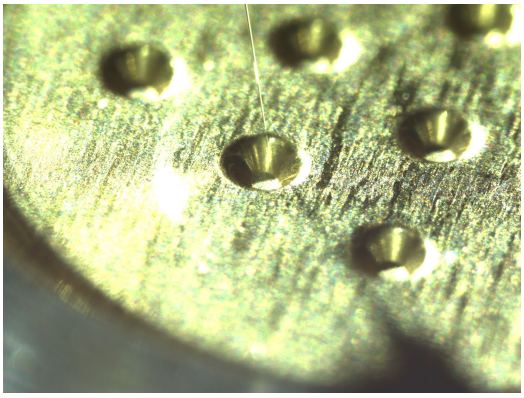

20200713/toAu13/nikon/03_MD03-G0620_releaseto_Au13s2.bmp

SAMPLE : RX-MD03-0224
PREID : MD03-G0620
PROCESS : release to Au13s2
OPERATOR : Yoshitake, Nishimura
COMMENT :

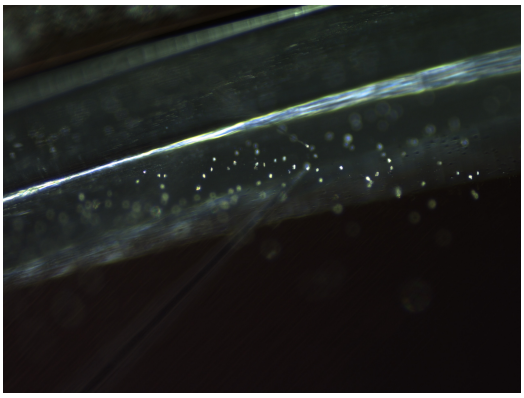

20200713/toAu13/nikon2/01_MD03-G0620_pickup.bmp

SAMPLE : RX-MD03-0224
PREID : MD03-G0620
PROCESS : pickup from MD03
OPERATOR : Yoshitake, Nishimura
COMMENT :

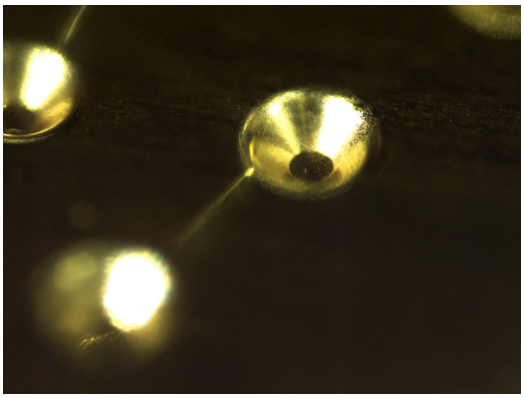

20200713/toAu13/nikon2/03_MD03-G0620_releaseto_Au13s2.bmp

SAMPLE : RX-MD03-0224
PREID : MD03-G0620
PROCESS : release to Au13s2
OPERATOR : Yoshitake, Nishimura
COMMENT :

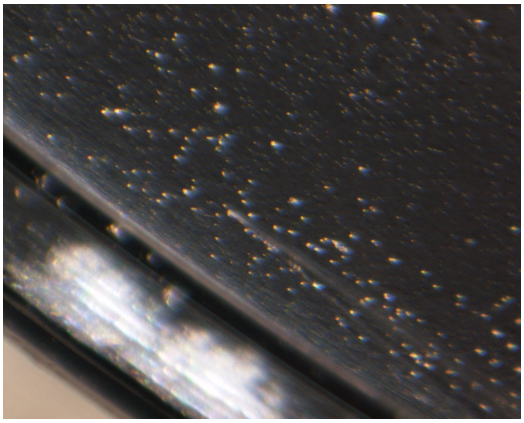

20200713/toAu13/union/01_MD03-G0620_pickup.bmp

SAMPLE : RX-MD03-0224
PREID : MD03-G0620
PROCESS : pickup from MD03
OPERATOR : Yoshitake, Nishimura
COMMENT :

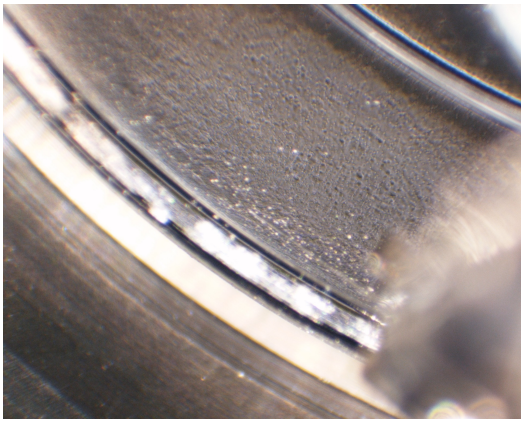

20200713/toAu13/union/02_MD03-G0620_pickup.bmp

SAMPLE : RX-MD03-0224
PREID : MD03-G0620
PROCESS : pickup from MD03
OPERATOR : Yoshitake, Nishimura
COMMENT :

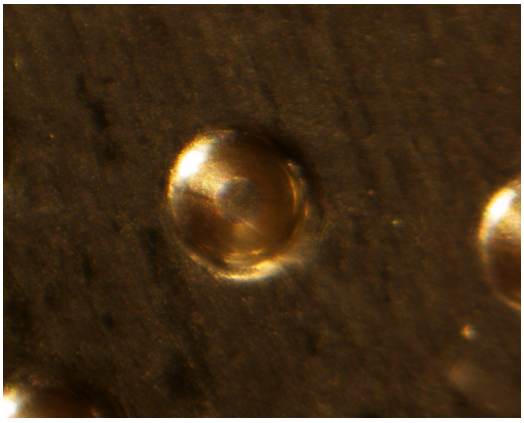

20200713/toAu13/union/03_MD03-G0620_releaseto_Au13s2.bmp

SAMPLE : RX-MD03-0224
PREID : MD03-G0620
PROCESS : release to Au13s2
OPERATOR : Yoshitake, Nishimura
COMMENT :

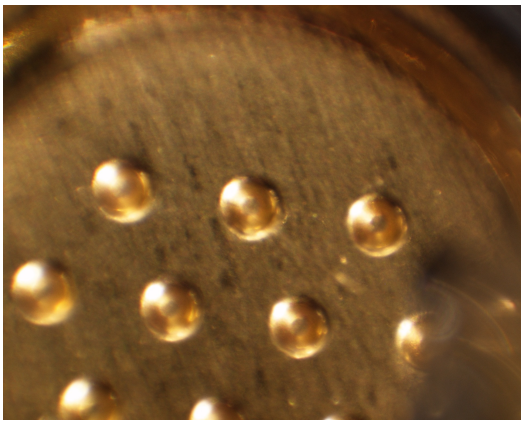

20200713/toAu13/union/04_MD03-G0620_releaseto_Au13s2.bmp

SAMPLE : RX-MD03-0224
PREID : MD03-G0620
PROCESS : release to Au13s2
OPERATOR : Yoshitake, Nishimura
COMMENT :

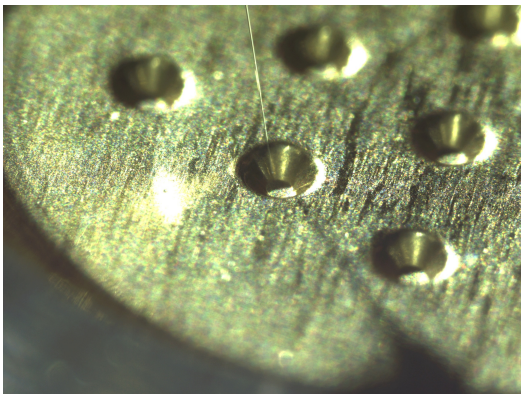

20200715/toSG45/nikon/03_MD03-G0620_pickupfromAu13s2.bmp

SAMPLE : RX-MD03-0224
PREID : MD03-G0620
PROCESS : pickup from Au13s2
OPERATOR : Yoshitake, Furuya
COMMENT :

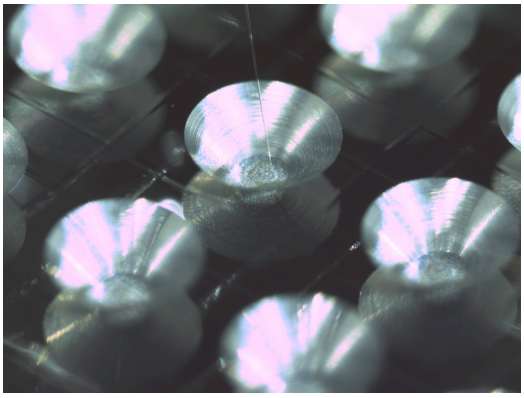

20200715/toSG45/nikon/05_MD03-G0620_releasetoSG45b2.bmp

SAMPLE : RX-MD03-0224
PREID : MD03-G0620
PROCESS : release to SG45b2
OPERATOR : Yoshitake, Furuya
COMMENT :

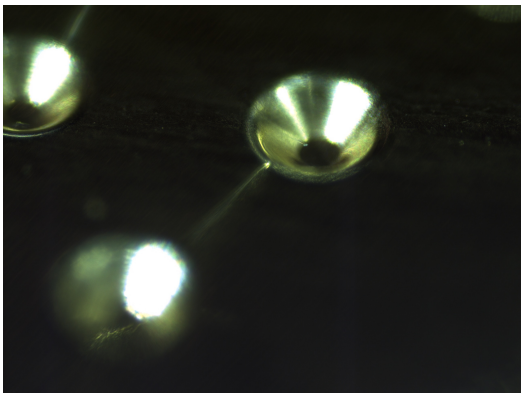

20200715/toSG45/nikon2/03_MD03-G0620_pickupfromAu13s2.bmp

SAMPLE : RX-MD03-0224
PREID : MD03-G0620
PROCESS : pickup from Au13s2
OPERATOR : Yoshitake, Furuya
COMMENT :

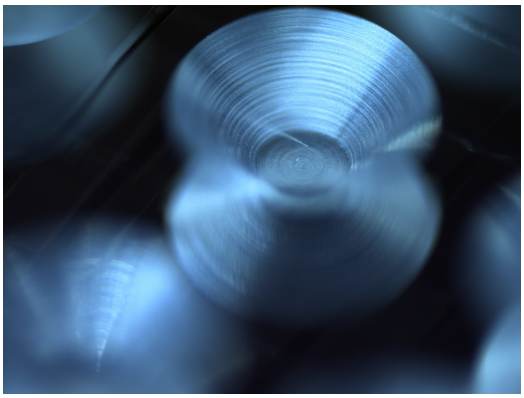

20200715/toSG45/nikon2/05_MD03-G0620_releasetoSG45b2.bmp

SAMPLE : RX-MD03-0224
PREID : MD03-G0620
PROCESS : release to SG45b2
OPERATOR : Yoshitake, Furuya
COMMENT :

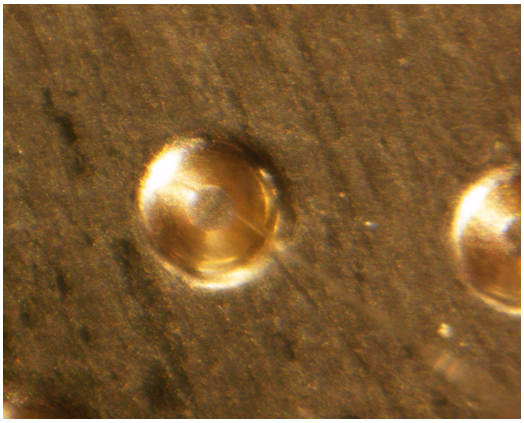

20200715/toSG45/union/03_MD03-G0620_pickupfromAu13s2.bmp

SAMPLE : RX-MD03-0224
PREID : MD03-G0620
PROCESS : pickup from Au13s2
OPERATOR : Yoshitake, Furuya
COMMENT :

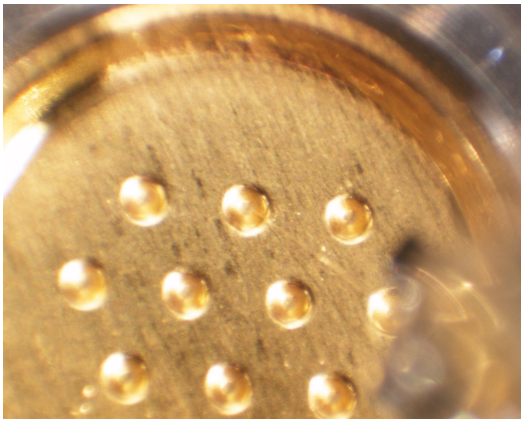

20200715/toSG45/union/04_MD03-G0620_pickupfromAu13s2.bmp

SAMPLE : RX-MD03-0224
PREID : MD03-G0620
PROCESS : pickup from Au13s2
OPERATOR : Yoshitake, Furuya
COMMENT :

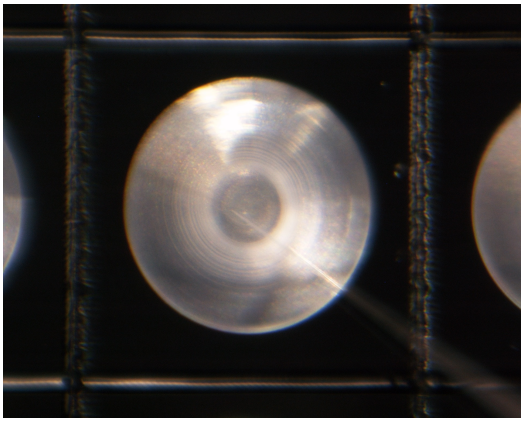

20200715/toSG45/union/05_MD03-G0620_releasetoSG45b2.bmp

SAMPLE : RX-MD03-0224
PREID : MD03-G0620
PROCESS : release to SG45b2
OPERATOR : Yoshitake, Furuya
COMMENT :

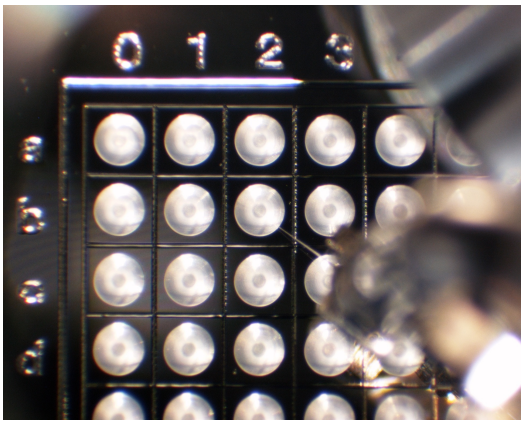

20200715/toSG45/union/06_MD03-G0620_releasetoSG45b2.bmp

SAMPLE : RX-MD03-0224
PREID : MD03-G0620
PROCESS : release to SG45b2
OPERATOR : Yoshitake, Furuya
COMMENT :

20220419/toS12/nikon/21_RX-MD03-0224_pickupfromSG45b2.bmp

SAMPLE : RX-MD03-0224
PREID :
PROCESS : pick up from SG45b2
OPERATOR : Soejima, Kanemaru
COMMENT :

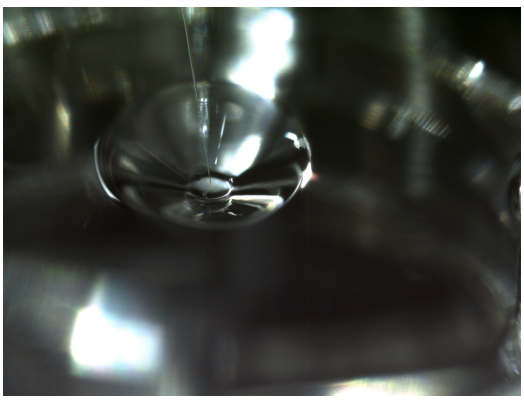

20220419/toS12/nikon/23_RX-MD03-0224_releasetoS12-225.bmp

SAMPLE : RX-MD03-0224
PREID :
PROCESS : release to S12-225
OPERATOR : Soejima, Kanemaru
COMMENT :

20220419/toS12/nikon2/21_RX-MD03-0224_pickupfromSG45b2.bmp

SAMPLE : RX-MD03-0224
PREID :
PROCESS : pick up from SG45b2
OPERATOR : Soejima, Kanemaru
COMMENT :

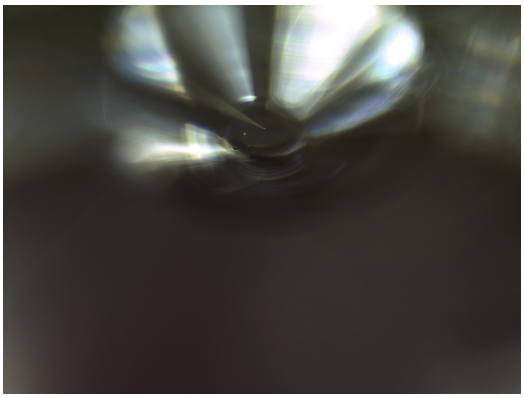

20220419/toS12/nikon2/23_RX-MD03-0224_releasetoS12-225.bmp

SAMPLE : RX-MD03-0224
PREID :
PROCESS : release to S12-225
OPERATOR : Soejima, Kanemaru
COMMENT :

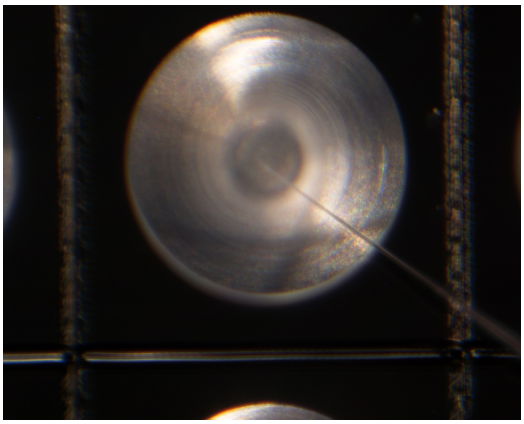

20220419/toS12/union/21_RX-MD03-0224_pickupfromSG45b2.bmp

SAMPLE : RX-MD03-0224
PREID :
PROCESS : pick up from SG45b2
OPERATOR : Soejima, Kanemaru
COMMENT :

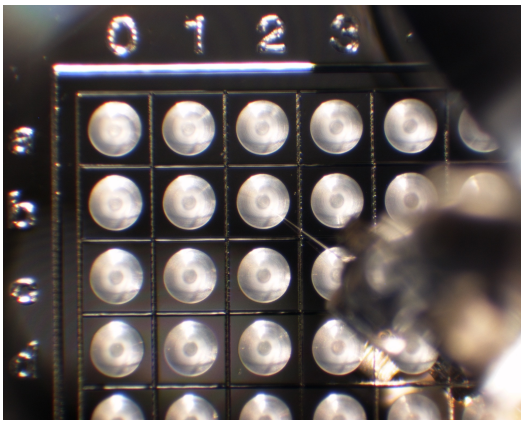

20220419/toS12/union/22_RX-MD03-0224_pickupfromSG45b2.bmp

SAMPLE : RX-MD03-0224
PREID :
PROCESS : pick up from SG45b2
OPERATOR : Soejima, Kanemaru
COMMENT :

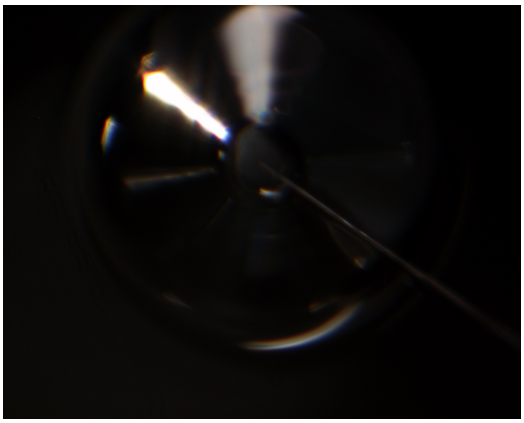

20220419/toS12/union/23_RX-MD03-0224_releasetoS12-225.bmp

SAMPLE : RX-MD03-0224
PREID :
PROCESS : release to S12-225
OPERATOR : Soejima, Kanemaru
COMMENT :

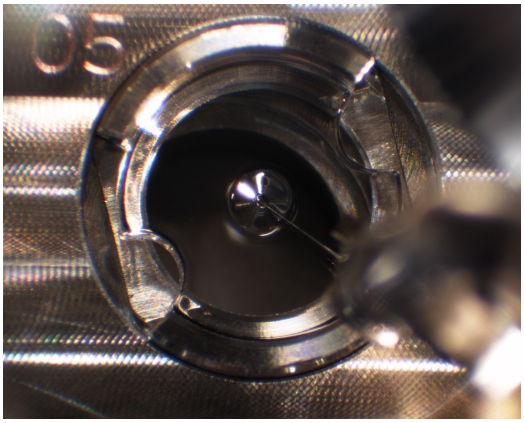

20220419/toS12/union/24_RX-MD03-0224_releasetoS12-225.bmp

SAMPLE : RX-MD03-0224
PREID :
PROCESS : release to S12-225
OPERATOR : Soejima, Kanemaru
COMMENT :

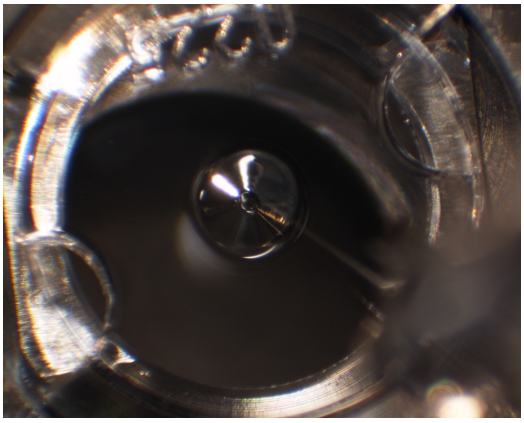

20220419/toS12/union/25_RX-MD03-0224_releasetoS12-225_covered.bmp

SAMPLE : RX-MD03-0224
PREID :
PROCESS : release to S12-225
OPERATOR : Soejima, Kanemaru
COMMENT : covered